# Viscosity measurement with the falling ball viscometer



Applied Science	Engineering	Applied Mechanics	Fluiddynamics & Aerodynamics
Difficulty level	<b>AA</b> Group size	<b>O</b> Preparation time	Execution time
hard	2	45+ minutes	45+ minutes

Your local Partner





Robert-Bosch-Breite 10 37079 Göttingen Tel.: 0551 604 - 0 Fax: 0551 604 - 107





# **General information**

# **Application**







Varnish

The viscocity of liquids is an important parameter in some industries, for example in:

- lubricants: a suitable lubricant is selected by its viscosity and how it varies with temperature
- medicine: viscosity of medications introduced into the body and the blood viscocity are critical factors in medicines.
- paints and varnishes: the thickness of liquids varies for different types of walls or furnitures



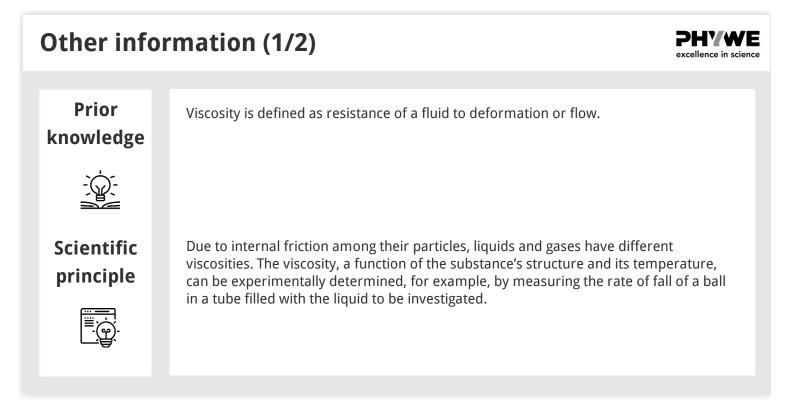

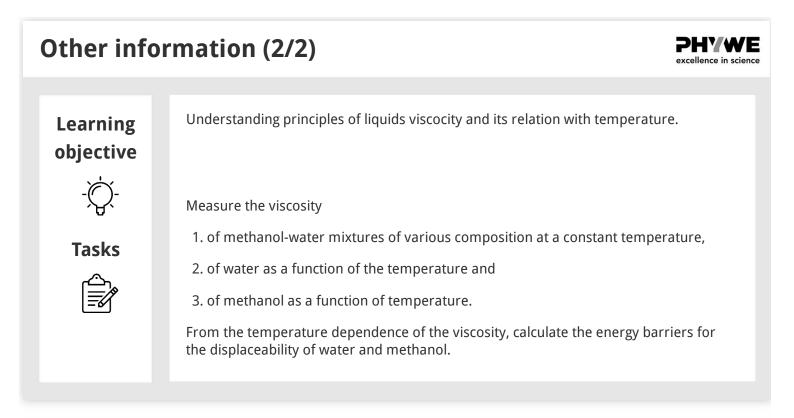

# **Safety instructions**

**PHYWE** excellence in science

For this experiment the general instructions for safe experimentation in science lessons apply.

For H- and P-phrases please consult the safety data sheet of the respective chemical.

# **Theory (1/6)**

The dynamic viscosity  $\eta$  of a liquid (1) is defined by the force F which is required to move two parallel layers of liquid both having the area A and separated by dx with the velocity  $d\omega$  with respect to each other.

$$\eta = \frac{F}{A \frac{d\omega}{dx}} \tag{1}$$

By relating the dynamic viscosity to the density  $\rho$  of the liquid, one obtains the kinematic viscosity v (2); the reciprocal of the dynamic viscosity is designated as fluidity  $\phi$  (3).

$$v = \frac{\eta}{
ho}$$
 (2)

$$\phi = \frac{1}{\eta} \tag{3}$$





PHYWE excellence in science

## **Theory (2/6)**

A spherical particle with a radius r moves in a liquid under the influence of a force F and the viscosity  $\eta$  with a constant velocity  $\omega$ .

$$\omega = \frac{F}{6\pi\eta r} \tag{4}$$

For the fall of a sphere in the gravitational field of the earth the motive force F is equal to the product of the acceleration of gravity g and the effective mass m, which can be expressed as the density difference between the sphere ( $\rho_1$ ) and the liquid ( $\rho_2$ ).

$$F = m'g = \frac{4}{3}\pi r^3 g(\rho_1 - \rho_2)$$
 (5)

The correlation (6) for the calculation of the viscosity, which is derived from (4) and (5), is only considered as the limit law for expanded media (the radius can be neglected with respect to that of the gravity tube); otherwise, the relationship can be approximated by corrections (Ladenburg Correction).

#### **Theory (3/6)**

$$\eta = \frac{2r^2 \left(\rho_1 - \rho_2\right)g}{g\omega} \tag{6}$$

For commercial falling ball viscometers with sets of calibrated spheres, the constants in equation (6) are combined with the apparative factors to form the spherical constant *K*; this makes the calculations much simpler:

$$\eta = Kt\left(\rho_1 - \rho_2\right) \tag{7}$$

(t = rate of fall of the sphere for a measuring distance of s = 100 mm)

The density  $\rho_2\,$  of the liquid at temperature T which is contained in Eq (7), can be calculated using the relationship



PHYWE excellence in science

# Theory (4/6)

 $\rho_2 = \frac{m}{V} \tag{8}$ 

(*m* = mass of the liquid; *V* = volume of the pycnometer)

using the experimentally determined pycnometer data or alternatively that obtained from Tables 1 and 2.

The viscosity is a function of the structure of the system and the temperature. The alteration in the measured viscosity in which the composition of methanol-water mixtures are expressed as the mass fraction  $\omega$  (9.1) or the mole fraction x (9.2) is an expression of the non-ideal behaviour of the liquids. It correlates to additional mixing phenomena such as mixing volume (volume contraction) and mixing enthalpy.

$$\omega_1=rac{m_1}{m_1+m_2}$$
 (9.1)

( $\omega_1$  = mass fraction,  $m_1$  = mass of the substance 1)

#### **Theory (5/6)**

$$x_1 = rac{n_1}{n_1 + n_2} = rac{rac{m_1}{M_1}}{rac{m_1}{M_1} + rac{m_2}{M_2}}$$
 (9.2)

(  $x_1$  = mole fraction,  $n_1$  quantity of substance,  $m_1$  = mass of the substance 1,  $M_1$  = molar mass of substance 1)

For many liquids the reduction of the viscosity with temperature is described by an empirically determined exponential function (10).

$$\frac{1}{\eta} = \phi = Ce - \frac{E}{RT}$$
(10)

 $R = 8.3144 \, J \cdot K^{-1} \cdot mol^{-1}$  , universal gas constant.

## Theory (6/6)

In this relationship which is analogous to the Arrhenius equation, C represents a system-dependent constant; E is an expression of the molar energy which is required to overcome the internal friction. This activation energy can be determined from the slope obtained by the linear relation (10.1) between  $ln \eta$  and 1/T

$$\ln \eta = \frac{E}{R} \frac{1}{T} - \ln C \tag{10.1}$$



www.phywe.de

#### Equipment


1         Falling ball viscometer         18220-00         1           2         Thermometer, 24+ 51 °C, for Falling ball viscometer         18220-02         1           3         Immersion thermostat Alpha A, 230 V         08493-93         1           4         Cooling coil for thermostat Alpha A         08493-01         1           5         External circulation set for thermostat Alpha A         08493-02         1           6         Bath for thermostat, makrolon         08487-02         1           7         Retort stand, h = 750 mm         37694-00         1           8         Right angle boss-head clamp         37697-00         1           9         Universal clamp with joint         37716-00         1           10         Pycnometer, calibrated, 25 ml         03023-00         1           11         Volumetric flask, Borosilicate, 100 ml, IGJ12/21         36548-00         9           12         Beaker, Borosilicate, all form, 150 ml         46032-00         11           13         Beaker, Borosilicate, all form, 250 ml         46054-00         1           14         Pasteur pipettes, 250 pcs         39275-03         1           15         Rubber tubing, i.d. 6 mm         39282-00         6 <td< th=""><th>Position</th><th>Material</th><th>Item No.</th><th>Quantity</th></td<>	Position	Material	Item No.	Quantity
3         Immersion thermostat Alpha A, 230 V         08493-93         1           4         Cooling coil for thermostat Alpha A         08493-01         1           5         External circulation set for thermostat Alpha A         08493-02         1           6         Bath for thermostat, makrolon         08487-02         1           7         Retort stand, h = 750 mm         37694-00         1           8         Right angle boss-head clamp         37697-00         1           9         Universal clamp with joint         37716-00         1           10         Pycnometer, calibrated, 25 ml         03023-00         1           11         Volumetric flask, Borosilicate, 100 ml, IGJ12/21         36548-00         9           12         Beaker, Borosilicate, tall form, 150 ml         46032-00         11           13         Beaker, Borosilicate, low form, 250 ml         36590-00         1           14         Pasteur pipettes, 250 pcs         36590-00         1           15         Rubber caps, 10 pcs         39275-03         1           16         Rubber tubing, i.d. 6 mm         39282-00         6           17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18	1	Falling ball viscometer	18220-00	1
4         Cooling coil for thermostat Alpha A         08493-01         1           5         External circulation set for thermostat Alpha A         08493-02         1           6         Bath for thermostat, makrolon         08487-02         1           7         Retort stand, h = 750 mm         37694-00         1           8         Right angle boss-head clamp         37697-00         1           9         Universal clamp with joint         37716-00         1           10         Pycnometer, calibrated, 25 ml         03023-00         1           11         Volumetric flask, Borosilicate, 100 ml, IGJ12/21         36548-00         9           12         Beaker, Borosilicate, tall form, 150 ml         46032-00         11           13         Beaker, Borosilicate, low form, 250 ml         46054-00         1           14         Pasteur pipettes, 250 pcs         36590-00         1           15         Rubber caps, 10 pcs         39275-03         1           16         Rubber tubing, i.d. 6 mm         39282-00         6           17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18         Wash bottle, plastic, 500 ml         33931-00         2           19	2	Thermometer, 24+ 51 °C, for Falling ball viscometer	18220-02	1
5         External circulation set for thermostat Alpha A         08493-02         1           6         Bath for thermostat, makrolon         08487-02         1           7         Retort stand, h = 750 mm         37694-00         1           8         Right angle boss-head clamp         37697-00         1           9         Universal clamp with joint         37716-00         1           10         Pycnometer, calibrated, 25 ml         03023-00         1           11         Volumetric flask, Borosilicate, 100 ml, IGJ12/21         36548-00         9           12         Beaker, Borosilicate, tall form, 150 ml         46032-00         11           13         Beaker, Borosilicate, low form, 250 ml         46054-00         1           14         Pasteur pipettes, 250 pcs         36590-00         1           15         Rubber caps, 10 pcs         39275-03         1           16         Rubber tubing, i.d. 6 mm         39282-00         6           17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18         Wash bottle, plastic, 500 ml         33931-00         2           19         Methanol 500 ml         31246-81         1           21         Hose clamp for 8-12	3	Immersion thermostat Alpha A, 230 V	08493-93	1
6         Bath for thermostat, makrolon         08487-02         1           7         Retort stand, h = 750 mm         37694-00         1           8         Right angle boss-head clamp         37697-00         1           9         Universal clamp with joint         37716-00         1           10         Pycnometer, calibrated, 25 ml         03023-00         1           11         Volumetric flask, Borosilicate, 100 ml, IGJ12/21         36548-00         9           12         Beaker, Borosilicate, tall form, 150 ml         46032-00         11           13         Beaker, Borosilicate, low form, 250 ml         46054-00         1           14         Pasteur pipettes, 250 pcs         36590-00         1           15         Rubber caps, 10 pcs         39275-03         1           16         Rubber tubing, i.d. 6 mm         39282-00         6           17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18         Wash bottle, plastic, 500 ml         33931-00         2           20         Water, distilled 5 l         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm <th>4</th> <th>Cooling coil for thermostat Alpha A</th> <th>08493-01</th> <th>1</th>	4	Cooling coil for thermostat Alpha A	08493-01	1
7       Retort stand, h = 750 mm       37694-00       1         8       Right angle boss-head clamp       37697-00       1         9       Universal clamp with joint       37716-00       1         10       Pycnometer, calibrated, 25 ml       03023-00       1         11       Volumetric flask, Borosilicate, 100 ml, IGJ12/21       36548-00       9         12       Beaker, Borosilicate, tall form, 150 ml       46032-00       11         13       Beaker, Borosilicate, low form, 250 ml       46054-00       1         14       Pasteur pipettes, 250 pcs       36590-00       1         15       Rubber caps, 10 pcs       39275-03       1         16       Rubber tubing, i.d. 6 mm       39282-00       6         17       Digital stopwatch, 24 h, 1/100 s and 1 s       24025-00       1         18       Wash bottle, plastic, 500 ml       33931-00       2         20       Water, distilled 5 l       31246-81       1         21       Hose clamp for 8-12 mm diameter       41000-00       10         22       Rubber tubing, i.d. 10 mm       39290-00       1	5	External circulation set for thermostat Alpha A	08493-02	1
8         Right angle boss-head clamp         37697-00         1           9         Universal clamp with joint         37716-00         1           10         Pycnometer, calibrated, 25 ml         03023-00         1           11         Volumetric flask, Borosilicate, 100 ml, IGJ12/21         36548-00         9           12         Beaker, Borosilicate, tall form, 150 ml         46032-00         11           13         Beaker, Borosilicate, low form, 250 ml         46054-00         1           14         Pasteur pipettes, 250 pcs         36590-00         1           15         Rubber caps, 10 pcs         39275-03         1           16         Rubber tubing, i.d. 6 mm         39282-00         6           17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18         Wash bottle, plastic, 500 ml         33931-00         2           19         Methanol 500 ml         30142-50         2           20         Water, distilled 5 l         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	6	Bath for thermostat, makrolon	08487-02	1
9       Universal clamp with joint       37716-00       1         10       Pycnometer, calibrated, 25 ml       03023-00       1         11       Volumetric flask, Borosilicate, 100 ml, IGJ12/21       36548-00       9         12       Beaker, Borosilicate, tall form, 150 ml       46032-00       11         13       Beaker, Borosilicate, low form, 250 ml       46054-00       1         14       Pasteur pipettes, 250 pcs       36590-00       1         15       Rubber caps, 10 pcs       39275-03       1         16       Rubber tubing, i.d. 6 mm       39282-00       6         17       Digital stopwatch, 24 h, 1/100 s and 1 s       24025-00       1         18       Wash bottle, plastic, 500 ml       33931-00       2         20       Water, distilled 5 l       31246-81       1         21       Hose clamp for 8-12 mm diameter       41000-00       10         22       Rubber tubing, i.d. 10 mm       39290-00       1	7	Retort stand, h = 750 mm	37694-00	1
10         Pycnometer, calibrated, 25 ml         03023-00         1           11         Volumetric flask, Borosilicate, 100 ml, IGJ12/21         36548-00         9           12         Beaker, Borosilicate, tall form, 150 ml         46032-00         11           13         Beaker, Borosilicate, low form, 250 ml         46054-00         1           14         Pasteur pipettes, 250 pcs         36590-00         1           15         Rubber caps, 10 pcs         39275-03         1           16         Rubber tubing, i.d. 6 mm         39282-00         6           17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18         Wash bottle, plastic, 500 ml         33931-00         2           20         Water, distilled 5 l         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	8	Right angle boss-head clamp	37697-00	1
11       Volumetric flask, Borosilicate, 100 ml, IGJ12/21       36548-00       9         12       Beaker, Borosilicate, tall form, 150 ml       46032-00       11         13       Beaker, Borosilicate, low form, 250 ml       46054-00       1         14       Pasteur pipettes, 250 pcs       36590-00       1         15       Rubber caps, 10 pcs       39275-03       1         16       Rubber tubing, i.d. 6 mm       39282-00       6         17       Digital stopwatch, 24 h, 1/100 s and 1 s       24025-00       1         18       Wash bottle, plastic, 500 ml       33931-00       2         19       Methanol 500 ml       30142-50       2         20       Water, distilled 5 l       31246-81       1         21       Hose clamp for 8-12 mm diameter       41000-00       10         22       Rubber tubing, i.d. 10 mm       39290-00       1	9	Universal clamp with joint	37716-00	1
12       Beaker, Borosilicate, tall form, 150 ml       46032-00       11         13       Beaker, Borosilicate, low form, 250 ml       46054-00       1         14       Pasteur pipettes, 250 pcs       36590-00       1         15       Rubber caps, 10 pcs       39275-03       1         16       Rubber tubing, i.d. 6 mm       39282-00       6         17       Digital stopwatch, 24 h, 1/100 s and 1 s       24025-00       1         18       Wash bottle, plastic, 500 ml       33931-00       2         19       Methanol 500 ml       30142-50       2         20       Water, distilled 5 l       31246-81       1         21       Hose clamp for 8-12 mm diameter       41000-00       10         22       Rubber tubing, i.d. 10 mm       39290-00       1	10	Pycnometer, calibrated, 25 ml	03023-00	1
13       Beaker, Borosilicate, low form, 250 ml       46054-00       1         14       Pasteur pipettes, 250 pcs       36590-00       1         15       Rubber caps, 10 pcs       39275-03       1         16       Rubber tubing, i.d. 6 mm       39282-00       6         17       Digital stopwatch, 24 h, 1/100 s and 1 s       24025-00       1         18       Wash bottle, plastic, 500 ml       33931-00       2         19       Methanol 500 ml       30142-50       2         20       Water, distilled 5 l       31246-81       1         21       Hose clamp for 8-12 mm diameter       41000-00       10         22       Rubber tubing, i.d. 10 mm       39290-00       1	11	Volumetric flask, Borosilicate, 100 ml, IGJ12/21	36548-00	9
14         Pasteur pipettes, 250 pcs         36590-00         1           15         Rubber caps, 10 pcs         39275-03         1           16         Rubber tubing, i.d. 6 mm         39282-00         6           17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18         Wash bottle, plastic, 500 ml         33931-00         2           19         Methanol 500 ml         30142-50         2           20         Water, distilled 5 l         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	12	Beaker, Borosilicate, tall form, 150 ml	46032-00	11
15       Rubber caps, 10 pcs       39275-03       1         16       Rubber tubing, i.d. 6 mm       39282-00       6         17       Digital stopwatch, 24 h, 1/100 s and 1 s       24025-00       1         18       Wash bottle, plastic, 500 ml       33931-00       2         19       Methanol 500 ml       30142-50       2         20       Water, distilled 5 l       31246-81       1         21       Hose clamp for 8-12 mm diameter       41000-00       10         22       Rubber tubing, i.d. 10 mm       39290-00       1	13	Beaker, Borosilicate, low form, 250 ml	46054-00	1
16         Rubber tubing, i.d. 6 mm         39282-00         6           17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18         Wash bottle, plastic, 500 ml         33931-00         2           19         Methanol 500 ml         30142-50         2           20         Water, distilled 5 l         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	14	Pasteur pipettes, 250 pcs	36590-00	1
17         Digital stopwatch, 24 h, 1/100 s and 1 s         24025-00         1           18         Wash bottle, plastic, 500 ml         33931-00         2           19         Methanol 500 ml         30142-50         2           20         Water, distilled 5 l         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	15	Rubber caps, 10 pcs	39275-03	1
18         Wash bottle, plastic, 500 ml         33931-00         2           19         Methanol 500 ml         30142-50         2           20         Water, distilled 5 l         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	16	Rubber tubing, i.d. 6 mm	39282-00	6
19         Methanol 500 ml         30142-50         2           20         Water, distilled 5 l         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	17	Digital stopwatch, 24 h, 1/100 s and 1 s	24025-00	1
20         Water, distilled 5 I         31246-81         1           21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	18	Wash bottle, plastic, 500 ml	33931-00	2
21         Hose clamp for 8-12 mm diameter         41000-00         10           22         Rubber tubing, i.d. 10 mm         39290-00         1	19	Methanol 500 ml	30142-50	2
22         Rubber tubing, i.d. 10 mm         39290-00         1	20	Water, distilled 5 I	31246-81	1
	21	Hose clamp for 8-12 mm diameter	41000-00	10
23         Tubing connector, ID 6-10mm         47516-01         2	22	Rubber tubing, i.d. 10 mm	39290-00	1
	23	Tubing connector, ID 6-10mm	47516-01	2





# Setup and procedure

#### Setup (1/2)

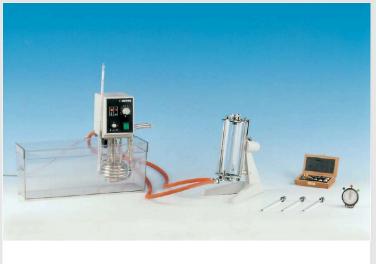

Experimental set-up

Perform the experimental set-up according to the figure. Connect the falling ball viscometer to the pump connection unit of the thermostat with rubber tubing (secure the tubing connections with hose clips!).

Fill the bath of the circulating thermostat with distilled or demineralised water to avoid furring.

Connect the cooling coil of the thermostat to the water supply line with tubing (secure the tubing connections with hose clips!).



PHYWE excellence in science

Setup (2/2)


$m( m CH_3OH)/ m g$	$m({ m H_2O})/{ m g}$	$ ho / { m g} \cdot { m cm}^{-3}$	$\eta/\mathrm{mPa}\cdot\mathrm{s}$
0	100	0.9970	0.897
10	90	0.9804	1.178
20	80	0.9649	1.419
30	70	0.9492	1.581
40	60	09316	1.671
50	50	0.9122	1.577
60	40	0.8910	1.427
70	30	0.8675	1.234
80	20	0.8424	1.025
90	10	0.8158	0.788
100	0	0.7867	0.557

Table 1

Prepare the falling ball viscometer according to its operating instructions; calibrate it; and for each experiment fill it with the liquid to be investigated (water, methanol or methanolwater mixtures according to the table) in such a manner that it is bubble-free.

Table 1: Literature values for the density and the dynamic viscosity of methanol-water mixtures of different compositions at constant temperature (T= 298.15 K)

# Procedure (1/2)



A constant working temperature of 298 K is recommended for the viscosity measurements in methanolwater mixtures (Tasks 1).

Conduct the investigations on the temperature dependence of the viscosity of pure liquids (Tasks 2 and 3) in steps of 5 K in the temperature range between 293 K and 323 K. Parallel to this, determine the density of the respective liquids, which is required for the calculations.

To do this, weigh the clean and dry pycnometer; fill it with the liquid to be investigated; fix it to the retort stand, and equilibrate it in the thermostatic water bath for approximately 15 minutes.



Robert-Bosch-Breite 10 37079 Göttingen

# Procedure (2/2)



PHYWE excellence in science


		Water		Methanol	
$T/{ m K}$	$ ho{=}/{ m g}\cdot{ m cm}^{-3}$	$\eta/\mathrm{mPa}\cdot\mathrm{s}$	$ ho / { m g} \cdot { m cm}^{-3}$	$\eta/\mathrm{mPa}\cdot\mathrm{s}$	
293.15	0.9982	1.002	0.7915	0.608	
298.15	0.9970	0.897	0.7868	0.557	
303.15	0.9956	0.797	0.7819	0.529	
308.15	0.9940	0.726	0.7774	0487	
313.15	0.9922	0.653	0.7729	0.458	
218.15	0.9902	0.597	0.7690	0.425	
323.15	0.9880	0.548	0.7650	0.396	

Subsequent to bubble-free closure with the accompanying stopper and a quick external drying, reweigh the filled pycnometer. From the mass difference of the two weighings and the volume of the pycnometer, determine the density of the liquid. Rinse the gravity tube and the pycnometer thoroughly with the next liquid to be investigated each time before it is refilled.

Table 2: Literature values for the density and the dynamic viscosity of water and methanol at different temperatures

Table 2

**Evaluation (1/5)** 

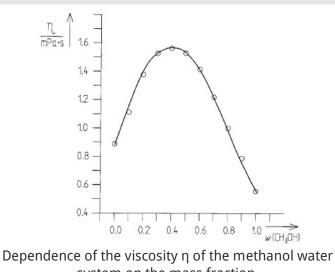

system on the mass fraction.

Figure shows the dependence of the viscosity  $\eta$  of the methanol water system on the composition described by the mass traction at constant temperature (T = 298 K).



**Evaluation (2/5)** 




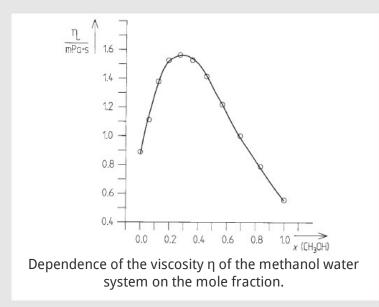


Figure shows the dependence of the viscosity  $\eta$  of the methanol water system on the composition described by the mole traction at constant temperature (T = 298 K).



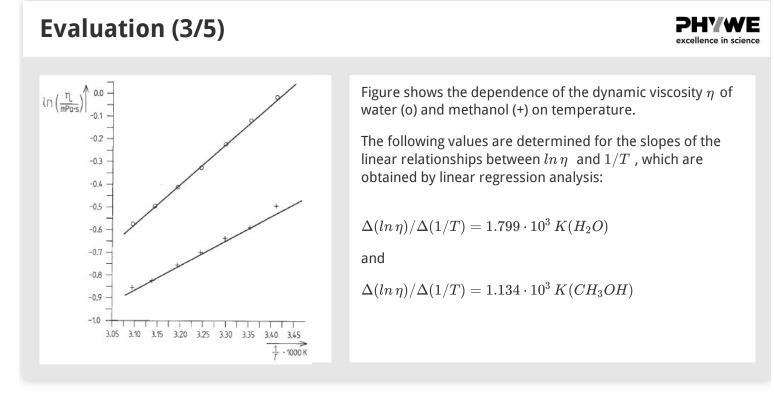

# **Evaluation (4/5)**

Substituting these values in Eq. (10.1), the corresponding energy barriers are obtained


 $E = 14.8 \, kJ \cdot mol^{-1} \, (H_2O)$  and

$$E = 9.4 \, kJ \cdot mol^{-1} \, (CH_3OH)$$

The energy barriers, which are obtained by using the literature values for  $\eta$  (given in Table 2), are

 $E=15.9\,kJ\cdot mol^{-1}$  and

 $E=11.1\,kJ\cdot mol^{-1}$ 

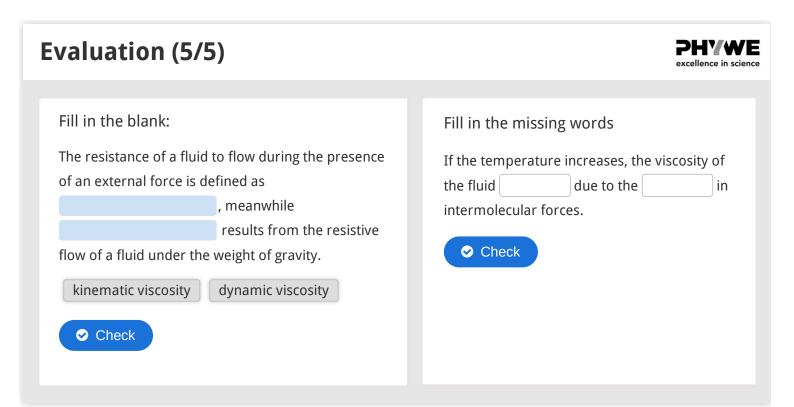



Slide		Score/Total
Slide 22: Multiple tasks		0/4
	Total Score	0/4
	Show solutions C Retry	